
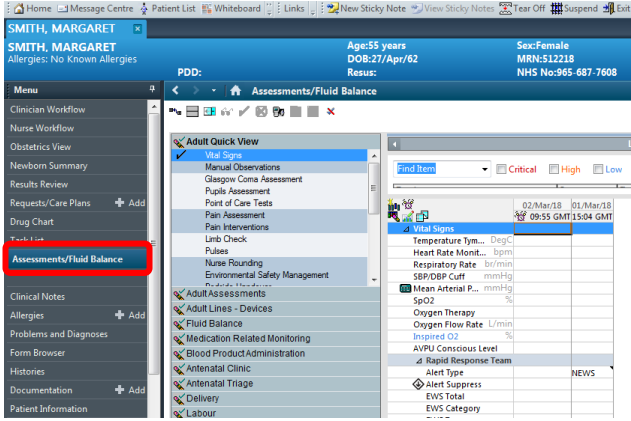
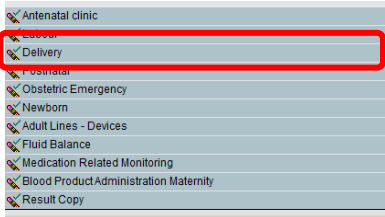
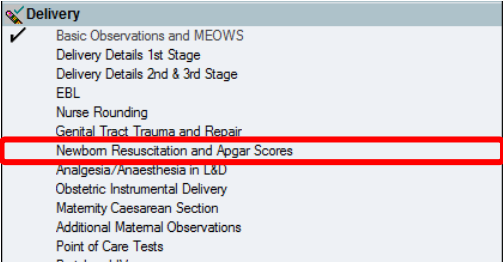
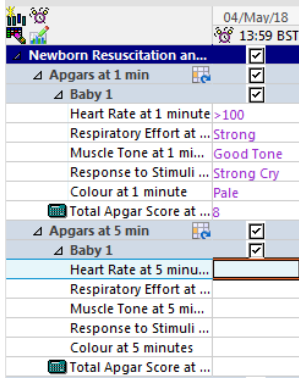


## RECORDING, CLEARING AND MODIFYING APGAR SCORE

<p>1.</p>	<p>Load up your patients record and and select the Assessments/Fluid Balance main menu option.</p> 
<p>2.</p>	<p>Select the Delivery iView band from the middle section.</p> 
<p>3.</p>	<p>Select Newborn Resuscitation and Apgar Scores</p> 
<p>4.</p>	<p>Double Click on the blue header to enable you to complete the apgar score for 1 minute 5 minutes and further.</p> 

5.

If you have made an error right click on the incorrect information and select Clear (this functionality is only available whilst the results haven't been signed).

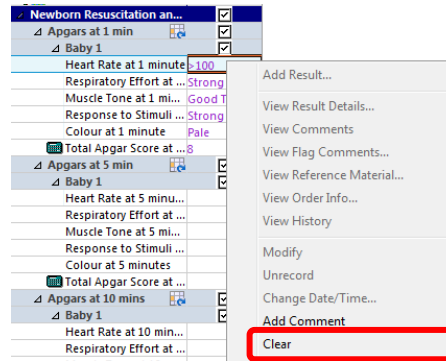


6.

Once you have completed then click on sign at the top of the bands.



7.

If you have made an error and signed, right click on the incorrect data and select Modify.

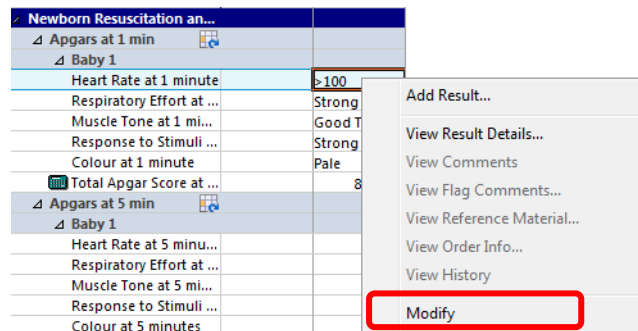

8.

You will need to click on sign again to confirm changes.



9.

The details will now show with a blue triangle to indicate this detail has been modified.

